

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property  
Organization  
International Bureau



(43) International Publication Date  
12 February 2004 (12.02.2004)

PCT

(10) International Publication Number  
WO 2004/012645 A1

(51) International Patent Classification<sup>7</sup>: A61H 39/00

(21) International Application Number:  
PCT/DK2003/000523

(22) International Filing Date: 5 August 2003 (05.08.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:  
PA 2002 01178 5 August 2002 (05.08.2002) DK

CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(71) Applicant and

(72) Inventor: WETLING, John, F. [DK/DK]; Peder Olsensvej 18, DK-3390 Hundested (DK).

Published:

— with international search report

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU,

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: ATMOSPHERIC ELECTRIC ACUPUNCTURE MONITOR

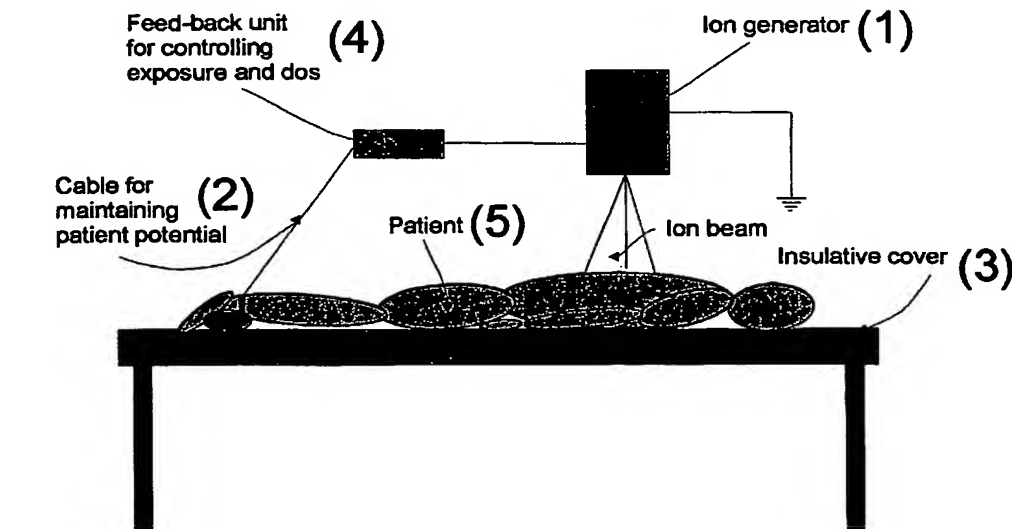


Diagram of the invention

(57) **Abstract:** Atmospheric electric acupuncture monitor, according to Fig. 5 consist of an ion generator (1) a feed back generator (4), connecting cables (2) and an insulative cover (3). The ion generator will deliver the ions to the object to be treated ( human or animal) resting on the insulative cover. The connecting cable will keep the object to be treated at a fixed potential ( usually zero with respect the ground). The feed back unit will monitor the exposure ( number of ions per unit time) as well as the total dose ( integrated charge) to the object. According to the invention it is possible to control the electric effect released by the ions plating out over the area exposed.

Best Available Copy

WO 2004/012645 A1